



23/02/2024 - 22/05/2024


# Compliance Report

Usage		23/02/2024 - 22/05/2024
Usage days	90/90 days (100%)	
>= 4 hours	88 days (98%)	
< 4 hours	2 days (2%)	
Usage hours	585 hours 39 minutes	
Average usage (total days)	6 hours 30 minutes	
Average usage (days used)	6 hours 30 minutes	
Median usage (days used)	6 hours 36 minutes	
Total used hours (value since last reset - 22/05/2024)	17,409 hours	

AirSense 10 Elite	
Serial number	23161959057
Mode	CPAP
Set pressure	7.2 cmH2O
EPR	Fulltime
EPR level	1

Therapy				
Leaks - L/min	Median:	0.0	95th percentile:	4.3
			Maximum:	8.6
Events per hour	AI:	1.1	HI:	0.2
			AHI:	1.3
Apnoea Index	Central:	0.0	Obstructive:	1.1
			Unknown:	0.0
Cheyne-Stokes respiration (average duration per night)				0 minutes (0%)

## Usage - hours

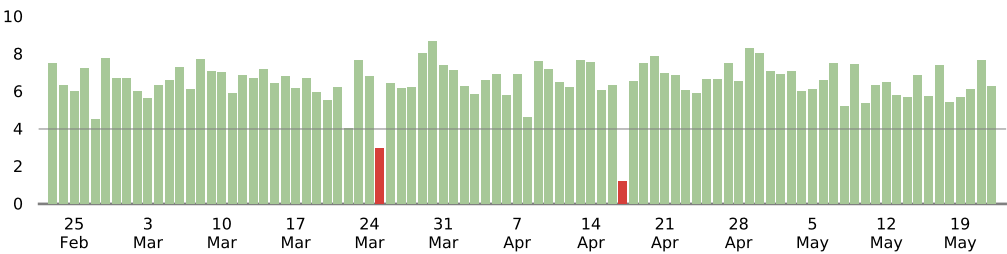




AirView™


Therapy Report

AirSense 10 Elite SN: 23161959057


Usage (hours)

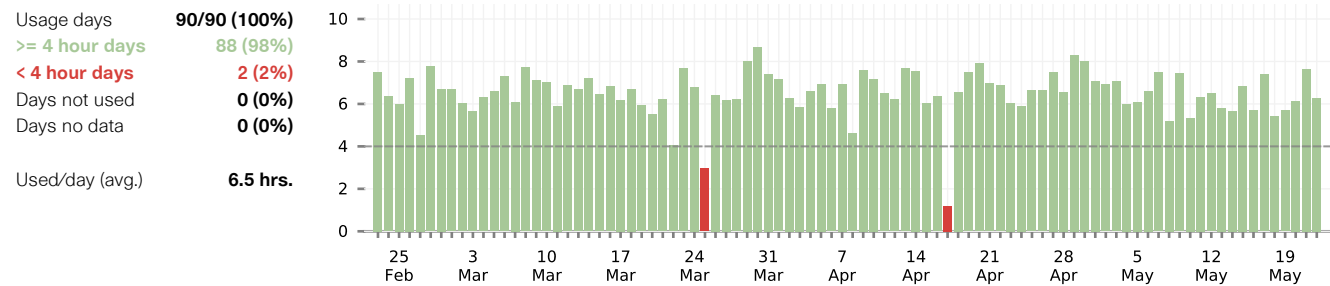

Leak (L/min)

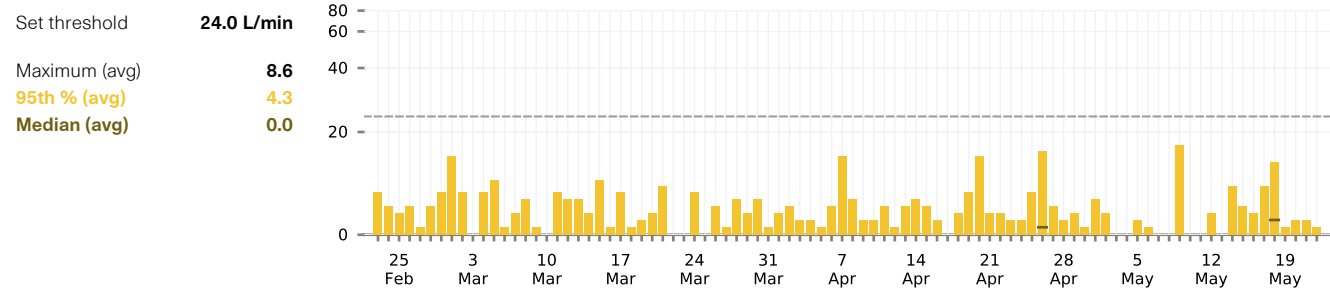

Pressure (cmH2O)

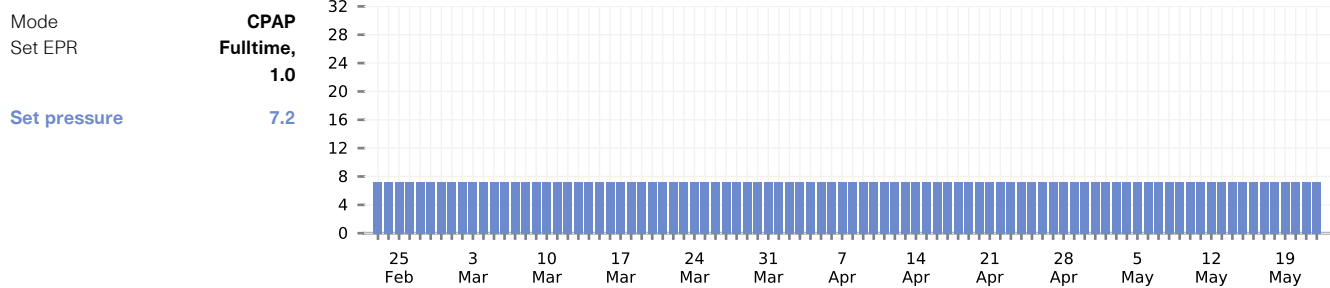

AHI (events/hour)

